


Myomatrix designs

- If you're reading this on a piece of paper, **measure the red lines**.
- If the lines are 1 and 10cm long as labeled, then the array schematics are the same size as the actual electrode arrays.
- If the red lines do NOT measure 1 and 10 cm, then the images are not life-sized (check to be sure you printed at 100% scale).
- Regardless, the **orange scale bar** is correct with respect to the array schematics.

Arrays for chronic or acute implantation

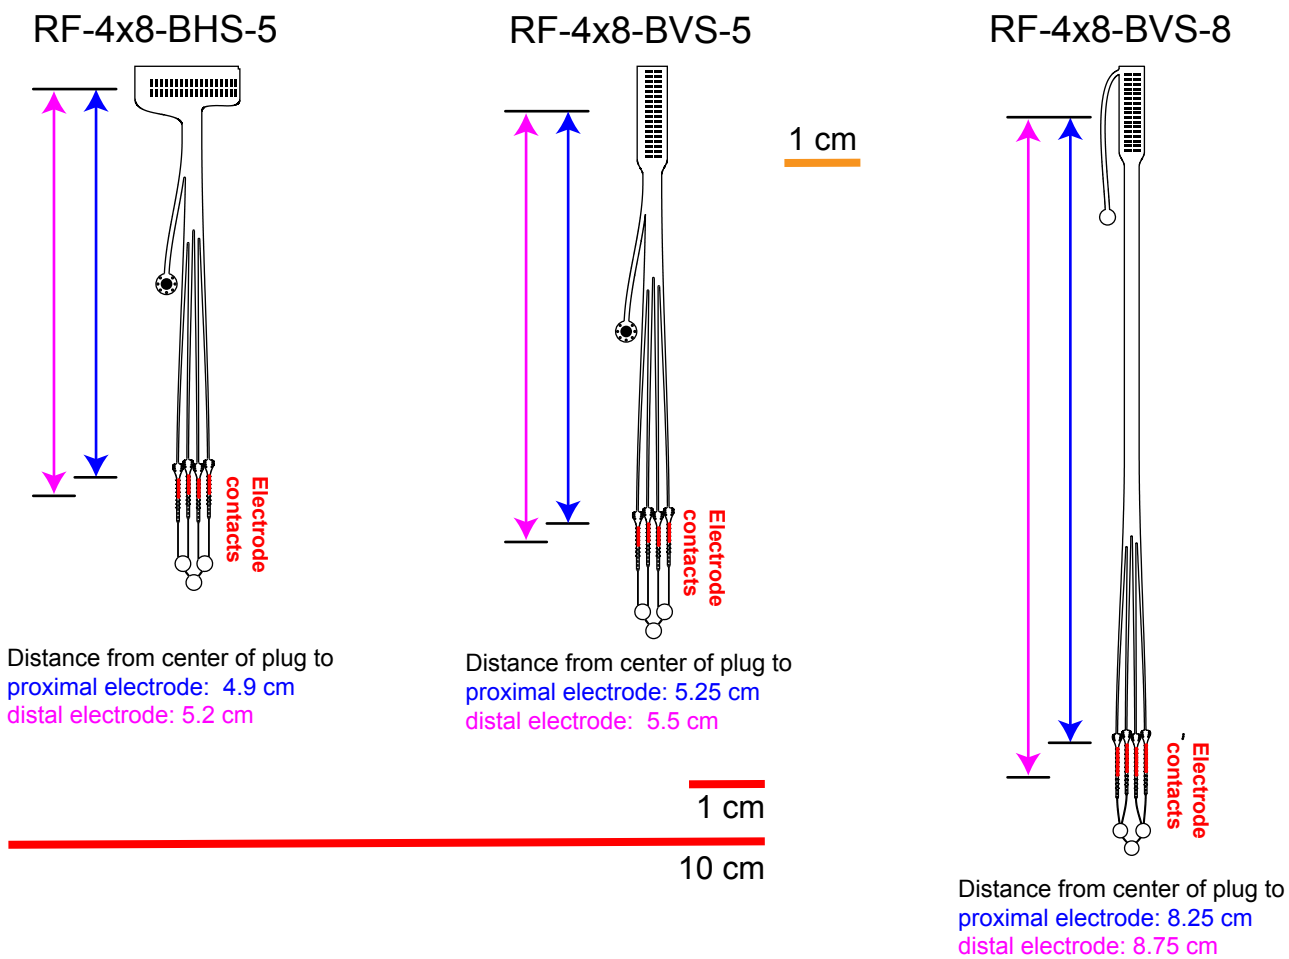

Arrays for percutaneous implantation

